



EdibleOil ICP

Heated & Fully Automated
Sample Introduction System
for Metals Analysis



The Missing Ingredient to Edible Oil Analysis



Time & Cost Savings

- Full multi-element analysis with little sample preparation
- Automatically melt & analyze a variety of sample types
- Free up scientists for more important tasks



Improved Results


- Improved detection limits by reducing dilution
- Greater stability & accuracy when analyzing sample types
- Excellent reproducibility



Fully Heated Flow Path

- Heats from sample deck to waste line
- Reduces sample viscosity
- Eliminates clogged lines from semiliquid and solid samples


EdibleOil ICP Features

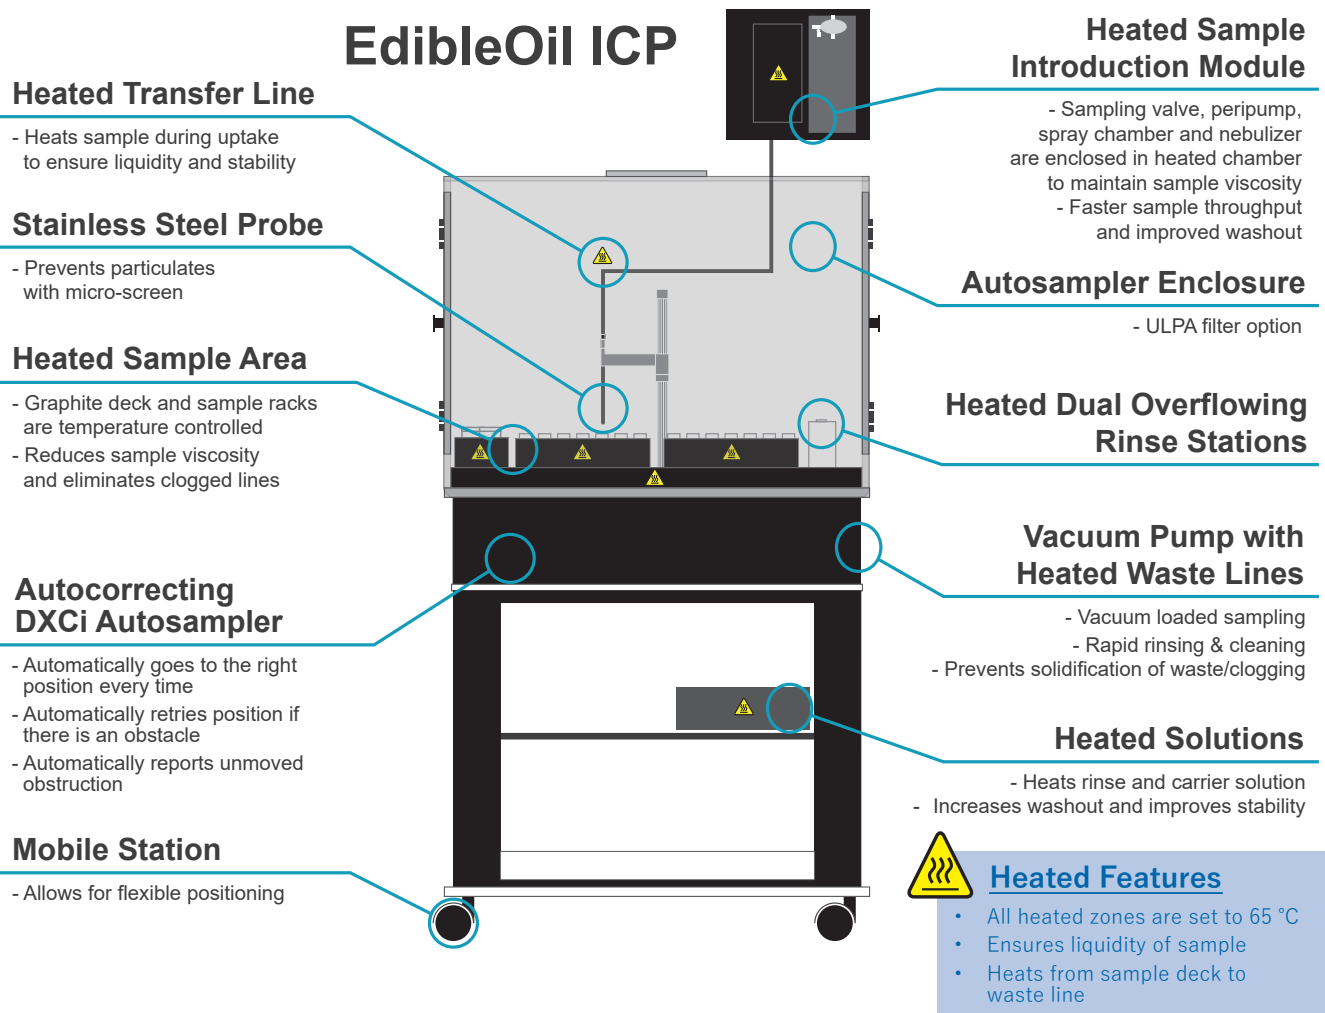

EdibleOil ICP – A Better Way to Analyze


Accuracy

EdibleOil ICP automates tedious manual labor and produces quality results for all kinds of edible oils and fats. The graph below shows ICP recovery of spiked sunflower oil samples prepared with a 7 ppm spike for all elements analyzed. Recovery for all elements ranged between 95-105%.

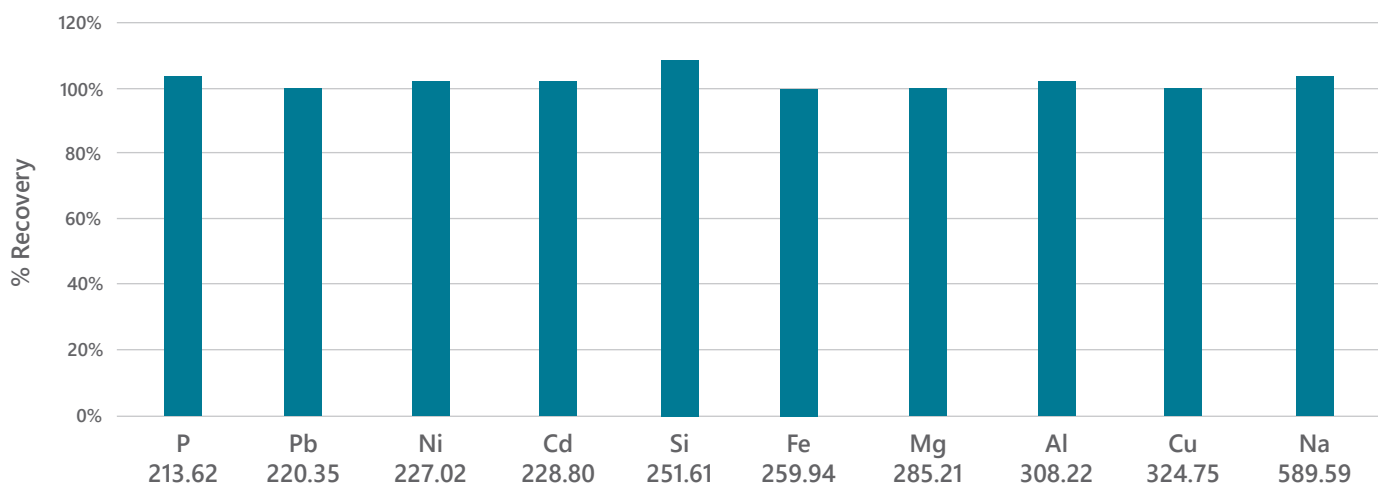

Stability

EdibleOil ICP's heating features prevent oils and fats from solidifying during analysis. Without sample path heating, palm stearin solidifies in seconds. The following stability data was collected over 11 hours using a solid palm stearin sample that was prepared by 1:1 dilution with V-Solv™ ICP Solvent containing 20 ppm Y. A 7 ppm spike was added to the sample for all ten elements in the table (right). The average %RSD for all 145 samples was 2.07%.

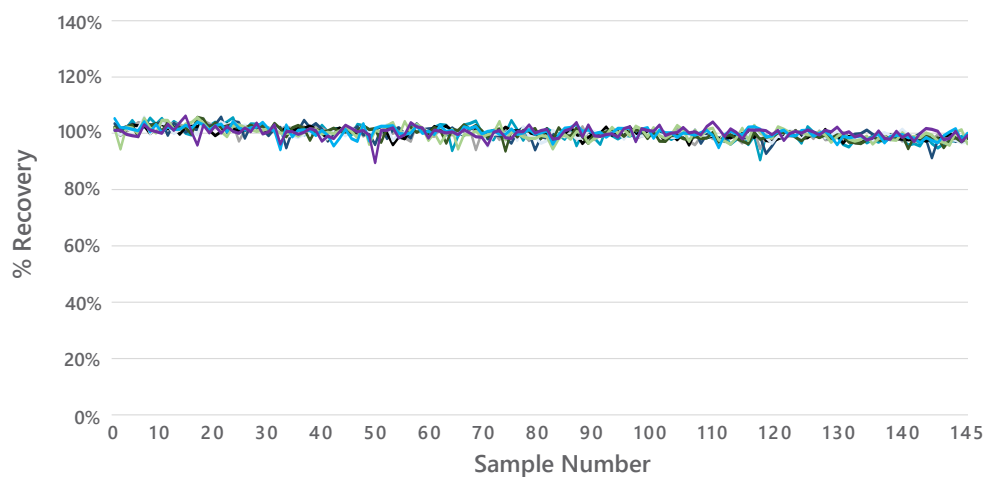



© Elemental Scientific | 7277 World Communications Drive | Omaha, NE 68122
Tel: 1-402-991-7800 | sales@icpms.com | www.icpms.com

B-22219-2