




FAST Automated Sample Introduction System


When you think productivity, think *FAST*!

FAST maximizes the productivity of the ICP-OES and ICPMS by optimizing and utilizing ALL of the non-productive steps in a sample acquisition

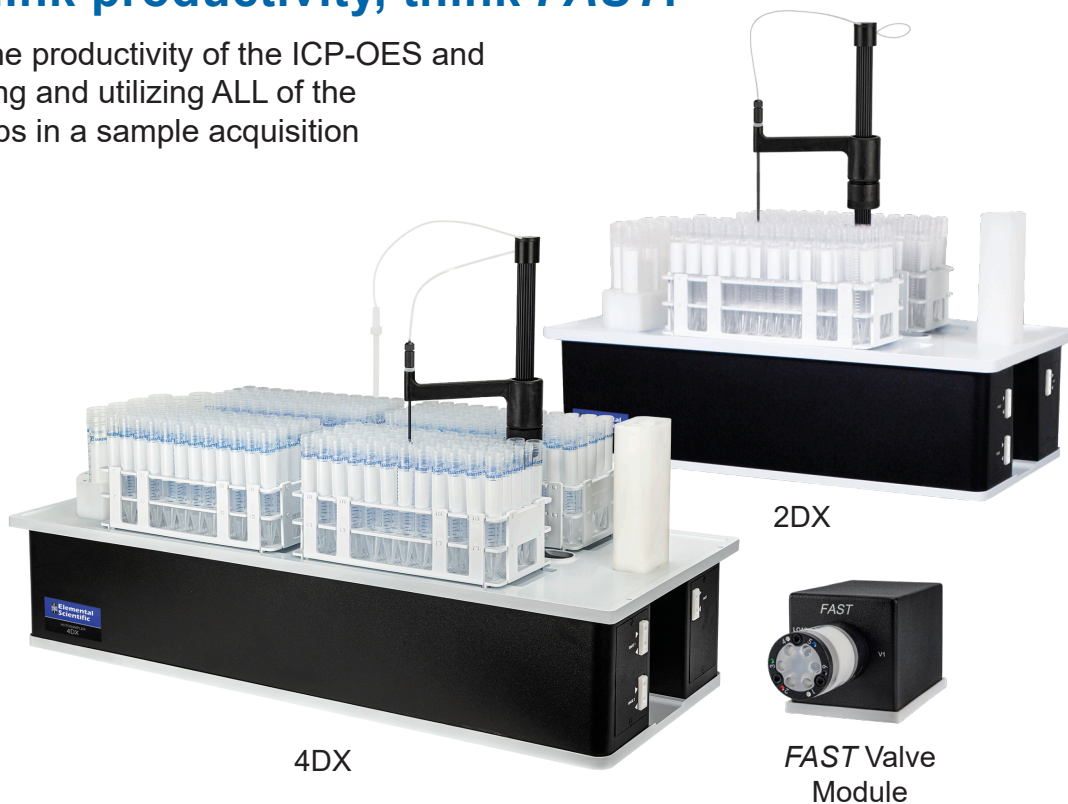


System Savings

- Lower reagent costst
 - Reduce concentration and volume of internal standard
 - Reduce sample volumes and reagents used to prepare samples
- Lower cost of consumables and routine maintenance
 - Shorter run times, lower consumption of power and Ar
 - Increase lifetime of Torch, Nebulizer, Cones, Pump (Oil), etc.
- Improved data quality
 - Fewer QC failures
 - Improved precision
 - Improved sensitivity
 - Lower oxides
 - Lower memory
 - Cleaner, faster washout reduces sample carry over
 - Dual rinse station improves rinse out and reduces blank contamination
- Optional precision micro peripump (MP²)
- High speed vacuum sample loading minimizes sample uptake time
- Available online internal standard addition
- Optional high speed and high precision syringe sample loading available
- Supports online dilution
- The sample never touches peripump tubing
 - Eliminates memory effects from pump tubing
- Compatible with virtually all ICP-OES/ICPMS systems
- Add volatile analytes such as Hg to ICPMS methods
- Pre-loaded FAST and ICP methods for rapid implementation
- Configurable for many applications

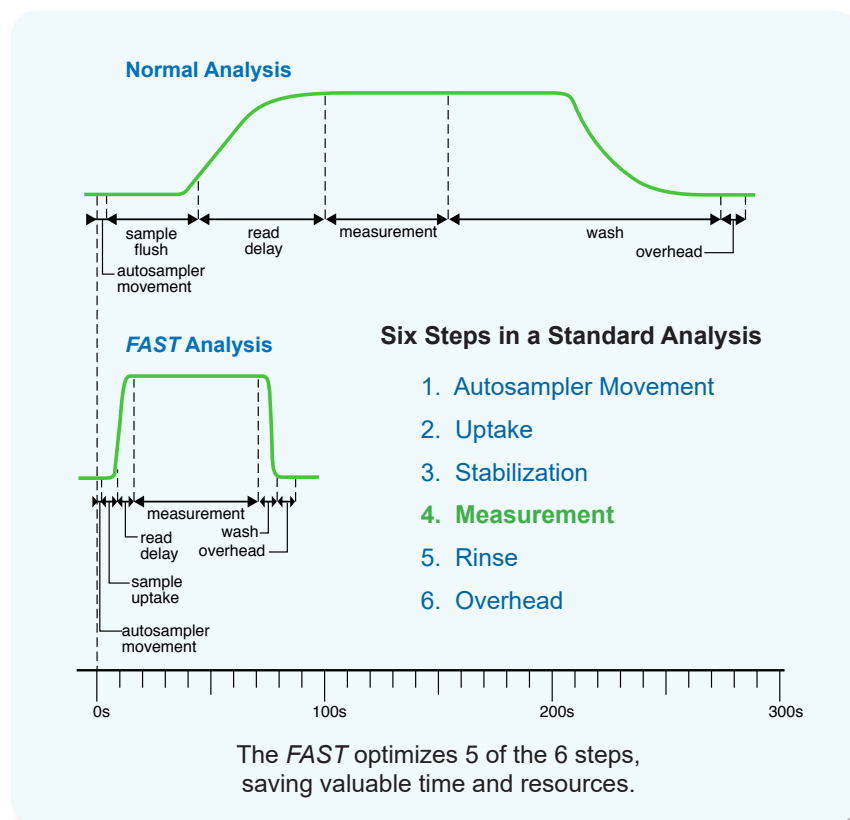

Unique Design

Utilizing a high flow vacuum pump, 6-port valve and ESI's SC-Software, the FAST is able to rapidly deliver the sample for analysis, saving valuable time. The unique design eliminates sample contact with peristaltic pump tubing, minimizing cross contamination. The peristaltic pump operates at a single, constant speed, further enhancing system stability. The FAST rinses the probe sample lines while the sample is being analyzed, making the FAST a true multi-tasking sample automated system.

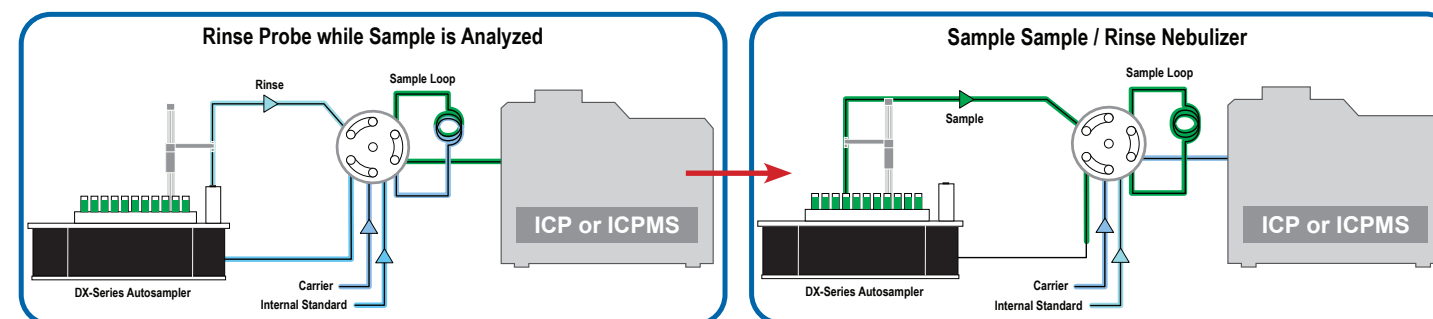

The FAST loads the sample loop as the nebulizer and tubing are being flushed.

And rinses the autosampler probe and tubing while the sample is being analyzed.



High Capacity 8DX

Table 1. Time Saving Comparisons

	Conventional	FAST
Sample Flush	30 (Sec)	8-10 (Sec)
Pump Speed	48 (RPM)	4 (RPM)
Read Delay	30 (Sec)	0 (Sec)
Pump Speed	10 (RPM)	4 (RPM)
Measurement	30 (Sec)	30 (Sec)
Pump Speed	12 (RPM)	4 (RPM)
Wash	45 (Sec)	5 (Sec)
Pump Speed	48 (RPM)	4 (RPM)
TOTAL TIME	135 (Sec)	43-45 (Sec)

This timing is typical when modifying an existing method for a FAST. The total time per sample has been reduced from 135 seconds to 45 seconds, with absolutely no compromise in data quality. The FAST analyzes 3 samples in the time it takes a conventional system to analyze one.

System	Sample Capacity			Microtiter-96 (2 mL)
	50 mL	15 mL	8 mL	
2DX (Super rack)	52 (64)	120 (160)	180	384
4DX	94	240	360	576
8DX	208	480	720	N/A
14DX	304	840	1260	2880



© Elemental Scientific | 7277 World Communications Drive | Omaha, NE 68122
Tel: 1-402-991-7800 | sales@icpms.com | www.icpms.com